

12

5.6.

AD

EDGEWOOD ARSENAL TECHNICAL REPORT

EC-TR-76068

A TRIGGER CIRCUIT FOR A HOT-WIRE-ANEMOMETER AEROSOL DETECTOR


by

William A. Cooper

Chemical Laboratory

October 1976

ADA030814



DEPARTMENT OF THE ARMY
Headquarters, Edgewood Arsenal
Aberdeen Proving Ground, Maryland 21010



Approved for public release; distribution unlimited.

Disclaimer

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

Disposition

Destroy this report when it is no longer needed. Do not return it to the originator.

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER 14 EC-TR-76068 ✓	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) 6 A TRIGGER CIRCUIT FOR A HOT-WIRE-ANEMOMETER AEROSOL DETECTOR		5. TYPE OF REPORT & PERIOD COVERED 7 Technical Report Jan 1976 - Mar 1977 6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) 10 William A. Cooper		8. CONTRACT OR GRANT NUMBER(s) 11 IW-762718-1-28742
9. PERFORMING ORGANIZATION NAME AND ADDRESS Commander, Edgewood Arsenal Attn: SAREA-CL-PO Aberdeen Proving Ground, MD 21010		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 16 DA - IW762718A084/02 AA AA
11. CONTROLLING OFFICE NAME AND ADDRESS Commander, Edgewood Arsenal Attn: SAREA-TS-R Aberdeen Proving Ground, MD 21010		12. REPORT DATE 11 Oct 1976
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) 12/12 P.		13. NUMBER OF PAGES 17
		15. SECURITY CLASS. (of this report) UNCLASSIFIED
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE NA
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release; distribution unlimited. Copies available from: NTIS, Springfield, Virginia 22151.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Electronics Hot wire anemometer Aerosol physics Aerosol challenge Aerosol concentration One-shot multivibrator Aerosol detector Electronic waveshaping		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) This report describes a cathode-coupled multivibrator which was designed and used in conjunction with a standard constant temperature anemometer (CTA) to measure local aerosol concentrations in turbulent impaction wind-tunnel experiments. The circuit acts like an electronic switch to actuate an electronic frequency counter each time a relatively cool aerosol particle impacts on a standard heating filament of the CTA and serves to prevent erroneous multiple counts from a single droplet.		

DD FORM 1473
1 JAN 73

EDITION OF 1 NOV 65 IS OBSOLETE

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

PREFACE

The work described in this report was authorized under Task 1W762718A084-02. This work was started in January 1971 and completed in March 1971. The experimental data are recorded in notebooks 8514 and 8531.

The use of trade names in this report does not constitute an official endorsement or approval of the use of such commercial hardware or software. This report may not be cited for purposes of advertisement.

Reproduction of this document in whole or part is prohibited except with permission of the Commander, Edgewood Arsenal, Attn: SAREA-TS-R, Aberdeen Proving Ground, Maryland 21010; however, DDC and the National Technical Information Service are authorized to reproduce the document for United States Government purposes.

CONTENTS

	<u>Page</u>
I. INTRODUCTION.....	5
II. BACKGROUND.....	6
III. DESIGN.....	7
IV. TESTING AND DISCUSSION.....	9
V. CONCLUSIONS.....	12
LITERATURE CITED.....	13
DISTRIBUTION LIST.....	15

LIST OF FIGURES

Figure

1	Configuration of Hot-Wire-Anemometer Aerosol-Detector System.....	6
2	Diagram of a Typical Cathode-Coupled Monostable Multivibrator....	7
3	Schematic of the Monostable Multivibrator Pulse Shaper.....	8
4	Output Pulse Width Versus RC Time Constant.....	8
5	Configuration of the Test Setup to Determine the Maximum Triggering Rate of the Multivibrator.....	9
6	Estimation of the Maximum Triggering Rate of the Multivibrator for Selected Pulse Widths.....	10
7	Estimation of Multiple Collisions or the Probable Error in Particle Count.....	11

A TRIGGER CIRCUIT FOR A HOT-WIRE-ANEMOMETER AEROSOL DETECTOR

I. INTRODUCTION.

The turbulent impaction of liquid particles on man-sized targets is a matter of great practical importance in chemical warfare offensive and defensive operations. Although certain cases of turbulent particle deposition can be formulated and analyzed mathematically, other potentially important deposition mechanisms are not amenable to rigorous mathematical treatment. To discern the mechanisms influencing the turbulent impaction of particles in these cases, experimental studies have been designed for representative bluff bodies (cylinders and sphere). These experiments are customarily performed in a controlled turbulent flow field produced in a wind tunnel. The effects of particle size distribution can then be studied effectively and synthesized by use of a variety of monometric (single-sized) and monodispersed particles.

The collection efficiency of a cylinder or sphere is defined by the fraction of the aerosol that is deposited on the bluff body in comparison with the total aerosol challenge. The total challenge is usually obtained by sampling the aerosol cloud by the so-called "isokinetic method" or by the impaction method. In both of these methods, the analysis and calibration are based on the assumption of laminar flow. It is expected that when turbulent flows prevail, quite different results are obtained which vary with the Reynolds number, the intensity of turbulence and the scale of turbulence, making the laminar results suspect for application to the case of turbulent flows.

Experimentally, the collecting material is usually a nondegradable absorbent paper, which must be removed from the sampling device and placed in a solvent as soon as possible after sample collection without loss of sample accuracy and then transported without degradation to a chemical laboratory for analysis. Additionally, an adequate description of the airborne fraction at low concentration levels, typical of wind tunnel-type dispersers, makes it necessary to sample for prolonged times in order to meet the sensitivity requirements of the spectrophotometric or colorimetric methods used in the chemical analysis.

A new method of measuring the local aerosol concentration in both laminar and turbulent flow conditions without the need for chemical analysis, extensive sample handling and time-consuming chemical analysis is the modified hot-wire-anemometer technique proposed by Goldschmidt¹ and Goldschmidt and Householder². A block diagram of a hot-filament aerosol detection technique is shown in figure 1. In this technique a standard heated sensor of a constant temperature anemometer (CTA) such as a fine tungsten wire or quartz-coated wire, is exposed to a turbulent air stream-laden with aerosol. The heated sensor undergoes temperature changes caused by the velocity fluctuations of the carrier air stream and also by losing heat to the relatively cold droplets which strike the heated filament. For the usual subsonic flows produced in a wind tunnel, most of the turbulent energy is contained in frequencies less than approximately 1 kHz, while the cooling signals resulting from the impaction of aerosol droplets on the heated

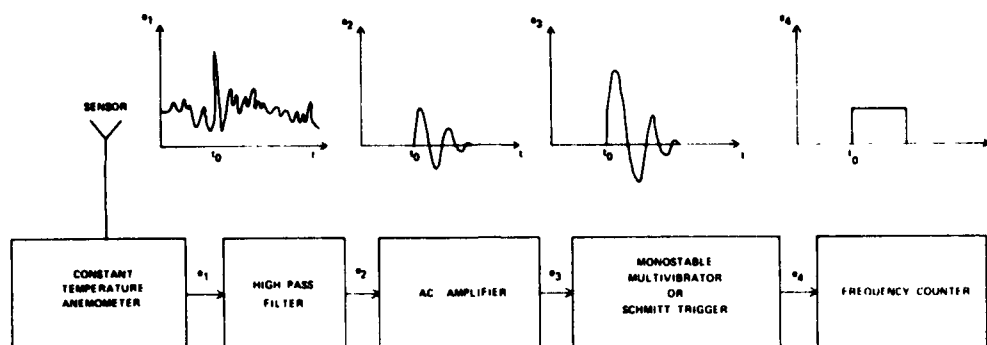


Figure 1. Configuration of Hot-Wire-Anemometer Aerosol- Detector System

filament display characteristic frequencies greater than 1 kHz. Therefore, the two effects can be discriminated by an appropriate high-pass frequency filter. Since the output of the filter is oscillatory by nature, it is necessary to eliminate these oscillations to prevent erroneous multiple counts for a single aerosol droplet impacting on the heated sensor. It is well known that a Schmitt trigger, or a one-shot multivibrator will produce pulses from some external source. If the pulse width of such a circuit is made equal to or longer than the oscillation time of the filter cooling signal, a countable pulse signal will be generated for each aerosol droplet impaction.

This report describes the design and testing of a one-shot or cathode-coupled multivibrator that will suitably perform the required waveshaping on the oscillatory cooling signal due to an aerosol droplet impaction.

II. BACKGROUND.

The basic one-shot or monostable multivibrator used to produce pulses, the duration of which is predetermined by circuit time constants, is shown in figure 2. The circuit is called a cathode-coupled monostable multivibrator since the cathodes are connected to a common cathode resistor, R_k . This circuit has the advantage that the triggering circuit is isolated from the multivibrator's output circuit by V_1 . The circuit has one stable and one semistable state. The bias applied by R_k is such that when there is no external trigger impulse applied to the grid of V_1 , it is cut off, so that the anode current of V_2 will be a maximum and the output voltage a minimum (the stable, quiescent state). On the arrival of a positive triggering impulse at the grid of V_1 , the tube will conduct for a period, T , its anode voltage will drop, and C_1 will be charged. Thus, a voltage negatively directed will be applied to the grid of V_2 which will drive V_2 beyond cutoff. The output voltage will rise to a maximum for a controlled period of time; that is until C_1 has discharged through R_3 . After this period of time, the circuit automatically returns to the stable condition and the output voltage drops to its minimum value.

The repetition-triggering rate of the circuit, or more appropriately, the particle-counting rate, is determined by T_p , the pulse width and T_R , the recovery or reset time of the multivibrator. A second output pulse cannot be started even if an input is applied, until V_1 has been restored to its nonconducting condition.

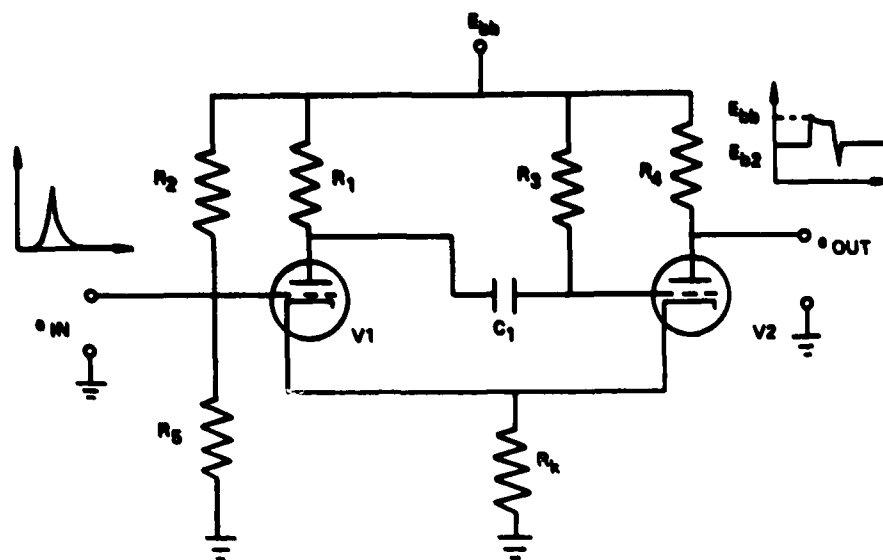


Figure 2. Diagram Of A Typical Cathode-Coupled Monostable Multivibrator

III. DESIGN

A schematic diagram of the cathode-coupled monostable multivibrator designed around a dual triode 6SN7 tube is shown in figure 3 which will be referred to throughout this section. Circuit values were generally selected in accordance with the principles outlined in Electronic Designers' Handbook by Landee, Davis and Albrecht.³ Sufficient stability in gate width and amplitude was obtained using standard 10-percent resistors; however, a substitution of a few different resistors for R_7 , R_8 and R_9 was required to insure that V1 is cut off when V2 is conducting as discussed in the previous section.

The filtered and amplified signals of the constant temperature anemometer are connected to the grid of V1 through coupling capacitor C_4 . V1 is normally cut off and V2 conducting but a positive voltage greater than approximately 8-volts peak will trip the circuit causing V1 and V2 to reverse roles for a predetermined period of time. Capacitors C_5 through C_{10} in conjunction with resistors R_{11} and R_{12} allow an adjustment of the duration of this time period from approximately 25 μ s to 10 ms, as shown in figure 4. The correspondence between the RC time constant of the circuit and the pulse width is given by the regression line $T_p = 0.512 TRC^{1.05}$. The variable resistor R_{13} provides an adjustable output pulse amplitude up to 20 volts peak which is clamped near the zero volt reference level by diode D_1 and R_6 . The power supply for the multivibrator circuit consists of transformer T1, full wave rectifier V3 (6X5), a RC filter network, R_1 , R_2 , R_3 and C_1 , C_2 , C_3 and two voltage regulators (VR150) V4 and V5. The ripple factor of the power supply is 0.002.

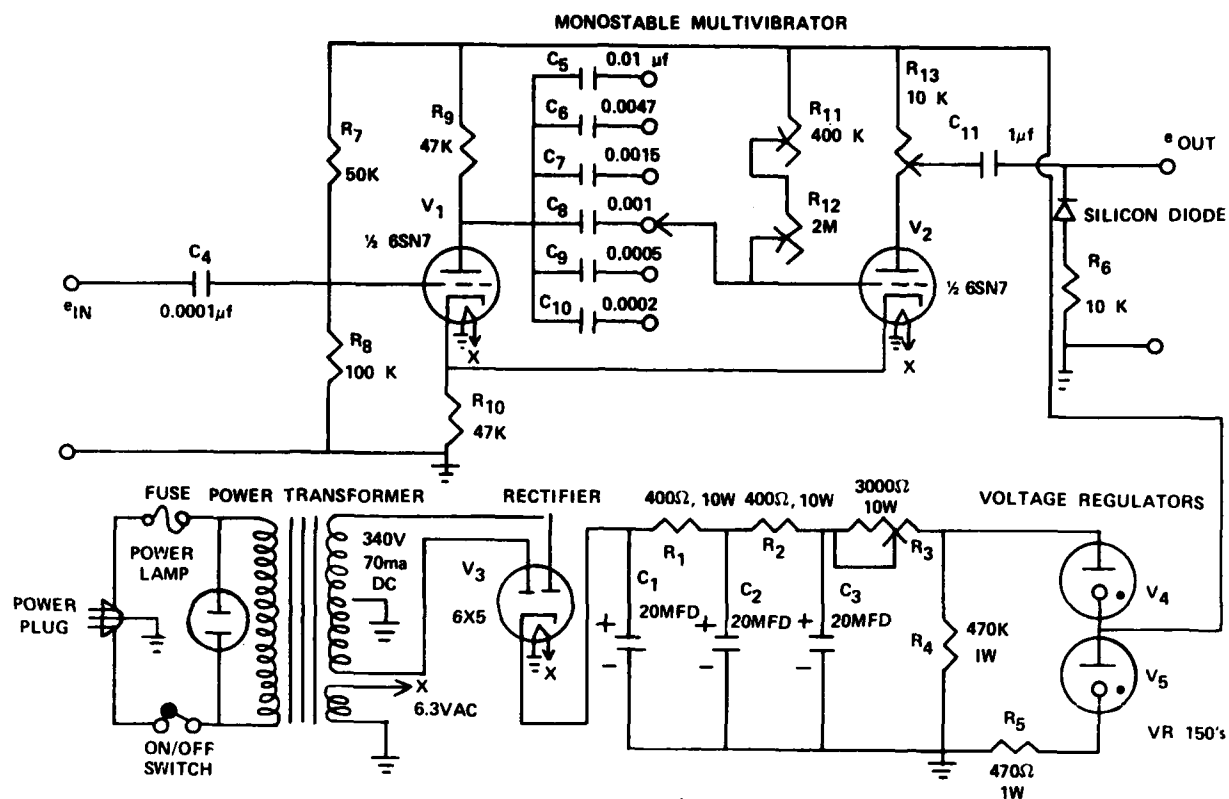


Figure 3. Schematic of the Monostable Multivibrator Pulse Shaper

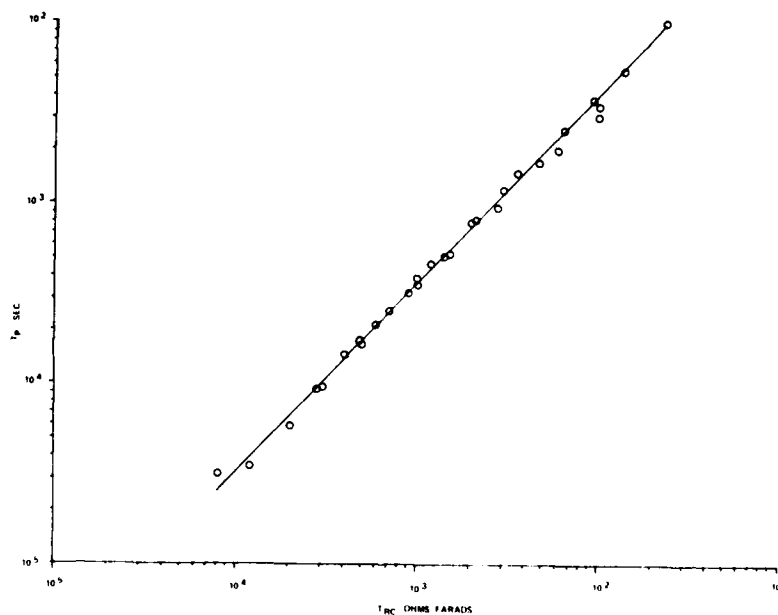


Figure 4. Output Pulse Width Versus RC Time Constant

IV. TESTING AND DISCUSSION

The maximum counting rate for the cathode-coupled multivibrator circuit for a particular RC time-constant selection was determined using the arrangement shown in figure 5. The external triggering signal was a train of short impulses obtained by differentiating a square pulse provided by an HP 3310A Function Generator. The frequency of this input signal was increased until the multivibrator failed to produce an output pulse of the same frequency and was then decreased until the one-to-one frequency correspondence was again achieved. Since some hysteresis was noticed, the "up-count" frequency was slightly larger than the "down-count" frequency. The lower value was used as an estimate of the maximum triggering rate of the circuit. The counting rate is plotted in figure 6 as a function of the output pulse width of the multivibrator. The test results indicate that, for a particular value of the timing capacitor, the frequency sensitivity of the multivibrator begins to decrease noticeably if the value of the timing resistor (R_{11}/R_{12}) is reduced below approximately $800k\Omega$. At this point, it is better to decrease the timing capacitor than the timing resistor. The straight line which corresponds to a duty cycle of 0.6 is, therefore, a conservative estimate of the maximum counting rate of the multivibrator when triggered by a periodic signal and, as shown, the rate can be varied from 10,000 events per second to 60 events per second for pulse widths of $60\mu s$ and 10 ms, respectively.

In reality, the physical event of liquid particles impacting on a small heated sensor of a constant temperature anemometer will not occur with ideal electrical response as does the periodic test signal used above. The collisions of the particles on the detector element will be random in nature and thus, the possibility exists that one, two or more droplets could strike the heated sensor simultaneously, that is during the time interval $T = T_p + T_r$ where T_p is the pulse width and T_r the reset time of the multivibrator. Such coincident events are not detected by the CTA aerosol sampler and could be a major source of error for certain test conditions.

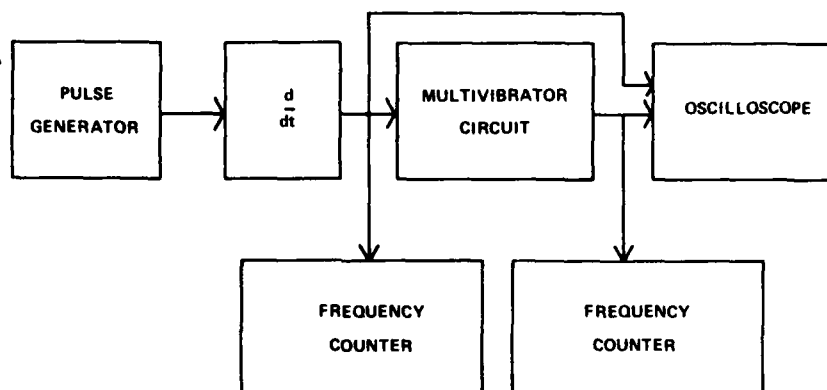


Figure 5. Configuration Of The Test Setup To Determine The Maximum Triggering Rate Of The Multivibrator

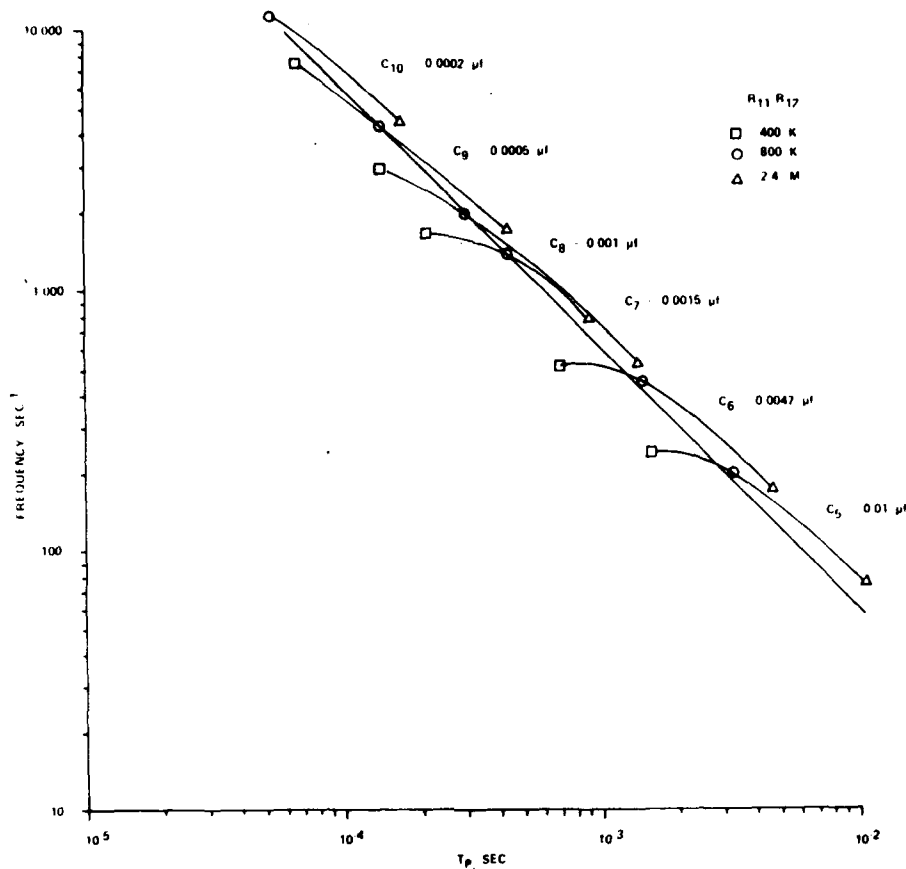


Figure 6. Estimation Of The Maximum Triggering Rate Of The Multivibrator For Selected Pulse Widths

However, it is reasonable to expect that the process satisfies the condition of a Poisson distribution, that is a collision occurs randomly on an average of λ times per second and the occurrence of n events in any time interval $(t_0, t_0 + \tau)$ is independent of the number of occurrences of the event before t_0 and depends only upon the length of the interval τ . Hence, the collision times are Poisson distributed and thus $P_K(\tau)$, the probability of K collision in τ seconds is given by

$$P_K(\tau) = \frac{(\lambda \tau)^K e^{-\lambda \tau}}{K!}$$

The probability of two or more collisions in a time interval τ for a collision density, λ , is then

$$\text{Prob} (K > 1; \lambda \tau) = 1 - P_0 - P_1$$

where P_0 is the probability of no collisions and P_1 is the probability of one collision in the time interval τ . Figure 7 shows the permissible particle collision rates that were calculated using the above relationship as a function of pulse width of the multivibrator for seven selected probability levels ranging from 0.0001 to 0.10. The results indicate that the probability of simultaneous collisions for low collision rates, typical of wind tunnel test conditions⁴, is very small and, therefore, the time response of the multivibrator should be more than adequate to measure accurately the aerosol drop-let challenge in such wind tunnel impaction experiments.

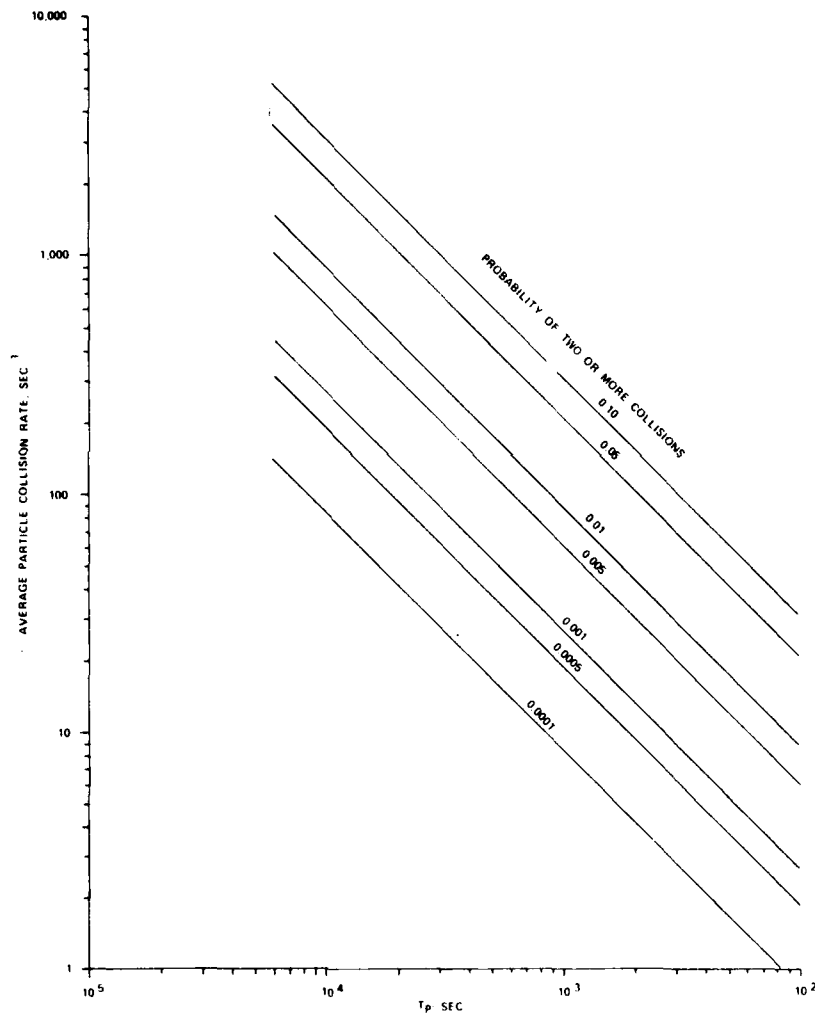


Figure 7. Estimation Of Multiple Collisions Or The Probable Error In Particle Count

V. CONCLUSIONS

A cathode-coupled multivibrator circuit was designed to produce pulses of a duration predetermined by circuit constants to facilitate counting the number of liquid particles striking a heated sensor of a constant temperature anemometer for measurement of the aerosol challenge in turbulent impaction experiments. Pulse duration of the multivibrator can be varied from $60 \mu s$ to 10 ms when triggered by an external impulse with an amplitude of 8-volts peak or greater and has a duty cycle of 0.6.

LITERATURE CITED

1. Goldschmidt, Victor W., Syracuse University. Contract DA-CML-18-108-61-G-27. The Sampling of Aerosols in Turbulent Air Flow. Progress Report No. 8. May 1962.
2. Goldschmidt, Victor W. and Householder, Michael K. Air Force Office of Scientific Research, Contract AF-AFOSR-1295-67. Measurements of Aerosols by Hot Wire Anemometry, Proceedings of the International Symposium on Hot Wire Anemometry. March 1967. (Held at University of Maryland, College Park, Maryland)
3. Landee, Robert W., Davis, Donovan C., and Albrecht, Albert P. Electronic Designers' Handbook. McGraw-Hill Book Company, Inc. New York, New York, 1957.
4. Stuenkel, A. K. EATR 4732. Impaction Efficiency of Cylindrical Collectors in Laminar and Turbulent Fluid Flow. March 1973.

DISTRIBUTION LIST 4

Names	Copies	Names	Copies
EDGEWOOD ARSENAL		Director	
TECHNICAL DIRECTOR		Defense Civil Preparedness Agency	
Attn: SAREA-TD-E	1	Attn: RE(DEP)	1
FOREIGN INTELLIGENCE OFFICER	1	Attn: PO(DC)	1
CHIEF, DEMILITARIZATION/DISPOSAL OFFICE	1	Washington, DC 20301	
CHIEF, LEGAL OFFICE	1	Commander-In-Chief	
CHIEF, SAFETY OFFICE	1	US Army Europe & 7A	
CDR, US ARMY TECHNICAL ESCORT CENTER	1	Attn: AEAGC-CNS	1
PUBLIC HEALTH SERVICE LO	8	APC New York 09403	
AUTHOR'S COPY, Chemical Laboratory	1	Chief, Office of Research,	
BIOMEDICAL LABORATORY		Development & Acquisition	
Attn: SAREA-BL-M	7	Attn: DAMA-CSM-CM	1
Attn: SAREA-BL-O	1	Attn: DAMA-ARZ-D	1
Attn: SAREA-BL-R	1	Washington, DC 20310	
Attn: SAREA-BL-RM	1	US Army Research and Standardization	
CHEMICAL LABORATORY		Group (Europe)	1
Attn: SAREA-CL-BS	1	Box 65, FPO New York 09510	
Attn: SAREA-CL-C	1	OFFICE OF THE SURGEON GENERAL	
Attn: SAREA-CL-P	1	HQDA (SGRD-EDE)	
Attn: SAREA-CL-T	1	Attn: LTC Charles Dettor	1
Attn: SAREA-CL-TE	1	WASH DC 20314	
DEVELOPMENT AND ENGINEERING DIRECTORATE		Commander	
Attn: SAREA-DE-S	1	US Army Research Institute of	
MANUFACTURING TECHNOLOGY DIRECTORATE		Environmental Medicine	
Attn: SAREA-MT-E	1	Attn: SGRD-UE-CA	1
DIRECTOR OF PRODUCT ASSURANCE		Natick, MA 01760	
Attn: SAREA-PA-P	1	Commander	
Attn: SAREA-PA-Q	1	US Army Medical Bioengineering	
DIRECTOR OF TECHNICAL SUPPORT		Research & Development Laboratory	
Attn: SAREA-TS-R	2	Attn: SGRD-UBD-AL	1
Attn: SAREA-TS-L	3	Fort Detrick, Bldg 568	
DEPARTMENT OF DEFENSE		Frederick, MD 21701	
Administrator		US ARMY HEALTH SERVICE COMMAND	
Defense Documentation Center		Commander	
Attn: Accessions Division	12	US Army Environmental Hygiene Agency	
Cameron Station		Attn: USAEHA-AL, Librarian, Bldg 2100	1
Alexandria, VA 22314		APG-Edgewood Area	
Director		Superintendent	
Defense Intelligence Agency		Academy of Health Sciences	
Attn: DIR-4G1	1	US Army	
Washington, DC 20301		Attn: AHS-CDC	1
DEPARTMENT OF THE ARMY		Attn: AHS-RHE	1
HQDA (DAMO-ODC)	1	Fort Sam Houston, TX 78234	
WASH DC 20310			

DISTRIBUTION LIST 4 (Contd)

Names	Copies	Names	Copies
US ARMY MATERIEL DEVELOPMENT AND READINESS COMMAND			
Commander US Army Materiel Development and Readiness Command Attn: DRCSF-C Attn: DRCDE-WB 5001 Eisenhower Ave Alexandria, VA 22333	1 1	Commandant US Army Missile & Munitions Center & School Attn: ATSK-TEB-E Redstone Arsenal, AL 35809	1
Commander US Army Foreign Science & Technology Center Attn: DRXST-IS1 220 Seventh St., NE Charlottesville, VA 22901	2	Commander US Army Armor School Attn: ATSB-CD-MS Fort Knox, KY 40121	1
Commander USAMC STIT-EUR APO New York 09710	1	Commander US Army Infantry School Attn: ATSH-CD-MS-C Fort Benning, GA 31905	1
Commander US Army Science & Technology Center-Far East Office APO San Francisco 96328	1	Commandant US Army Ordnance Center & School Attn: ATSL-CTD-MS-C APG-Aberdeen Area	1
Project Manager for Chemical Demilitarization and Installation Restoration Attn: DRCPM-DR APG-Edgewood Area	1	US ARMY TEST & EVALUATION COMMAND	
US ARMY ARMAMENT COMMAND		Record Copy CDR, APG Attn: STEAP-AD-R/RHA APG-Edgewood Area, Bldg E5179	1
Commander US Army Armament Command Attn: DRSAR-ASH Attn: DRSAR-RDT Attn: DRSAR-SA Rock Island, IL 61201	1 1 1	CDR, APG Attn: STEAP-TL APG-Aberdeen Area Commander US Army Test & Evaluation Command Attn: AMSTE-NB APG-Aberdeen Area	1 1 1
Commander Pine Bluff Arsenal Attn: SARP-B-ETA Pine Bluff, AR 71611		Commander US Army Tropic Test Center Attn: STETC-MO-A (Tech Library) APO New York 09827	1
Commander Frankford Arsenal Attn: Library Branch, TSP-L Bldg 51-2 Philadelphia, PA 19137	1	Commander Dugway Proving Ground Attn: STEDP-PC Dugway, UT 84022	1
US ARMY TRAINING & DOCTRINE COMMAND		DEPARTMENT OF THE NAVY	
Commandant US Army Infantry School Combat Support & Maintenance Dept. Attn: NBC Division Fort Benning, GA 31905	1	Chief of Naval Research Attn: Code 443 800 N. Quincy Street Arlington, VA 22209	1
		Commander Naval Surface Weapons Center White Oak Laboratory Silver Spring, MD 20910	1

DISTRIBUTION LIST 4 (Contd)

Names	Copies	Names	Copies
Commander Naval Intelligence Support Center 4301 Suitland Road Washington, DC 20390	1	OUTSIDE AGENCIES	
Commander Naval Surface Weapons Center Dahlgren Laboratory Attn: GFC Dahlgren, VA 22448		Director of Toxicology National Research Council 2101 Constitution Ave, NW Washington, DC 20418	1
Commander Nuclear Weapons Training Group-Atlantic Attn: Nuclear Warfare Department Norfolk, VA 23511	1	Director Central Intelligence Agency Attn: ORD/DD/S&T Washington, DC 20505	1
Chief, Bureau of Medicine & Surgery Department of the Navy Attn: CODE 553-1 Washington, DC 20372	1		
Commander Naval Air Systems Command Attn: Code AIR-350E Attn: Code AIR-53231B Washington, DC 20361	1 1		
Commanding Officer Naval Weapons Support Center Attn: Code 5042/Dr. B. E. Doua Crane, IN 47522	1		
DEPARTMENT OF THE AIR FORCE			
HQ Foreign Technology Division (AFSC) Attn: PDTR-3 Wright-Patterson AFB, OH 45433	1		
Commander Aeronautical Systems Division Attn: ASD/AELD Wright-Patterson AFB, OH 45433	1		
HQ, USAF/SCPR Forrestal Bldg WASH DC 20314	1		
HQ, Ogden ALC/MMWRAT Hill AFB, UT 84406	1		
Director Air Force Inspection and Safety Center Attn: IGD(AFISC/SEV) Norton AFB, CA 92409	1		